

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS


IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**




TITLE: HANDLE FOR ENDOSCOPIC DEVICE
FIRST NAMED INVENTOR: Christopher Hess
APP#:
ATTY: Gerry Gressel TEL. #: 513-337-3535
DOCKET #: END-5212 CUST. #: 000027777

1/14

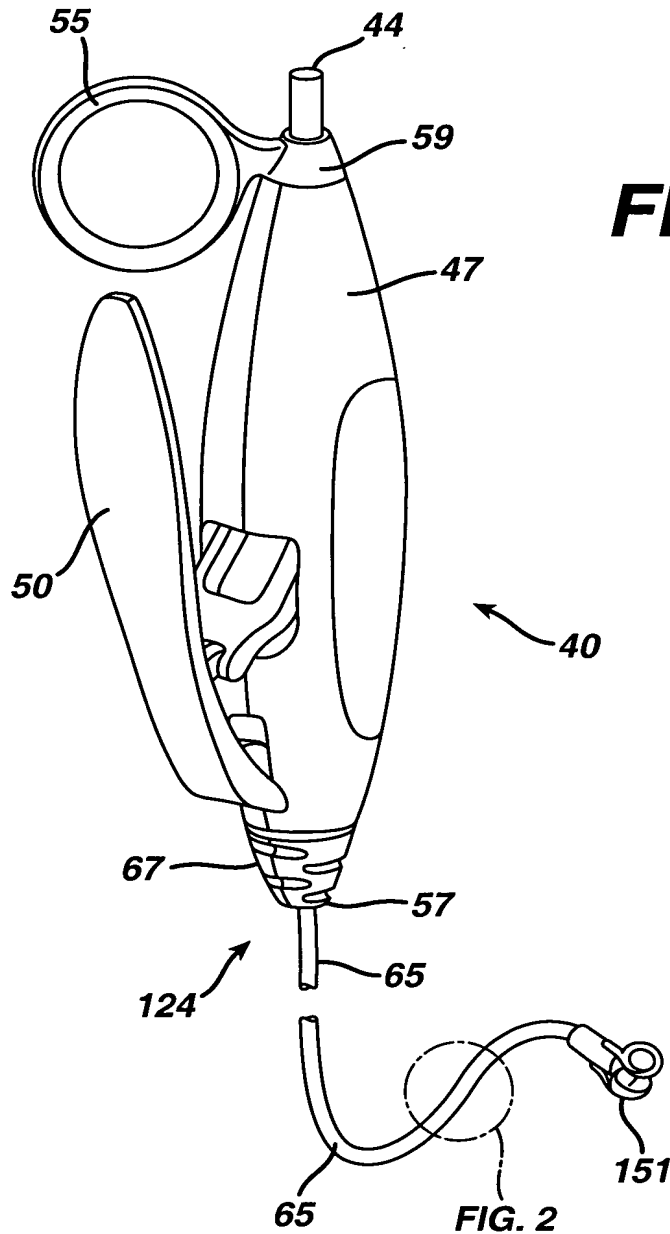


2/14


FIG. 2



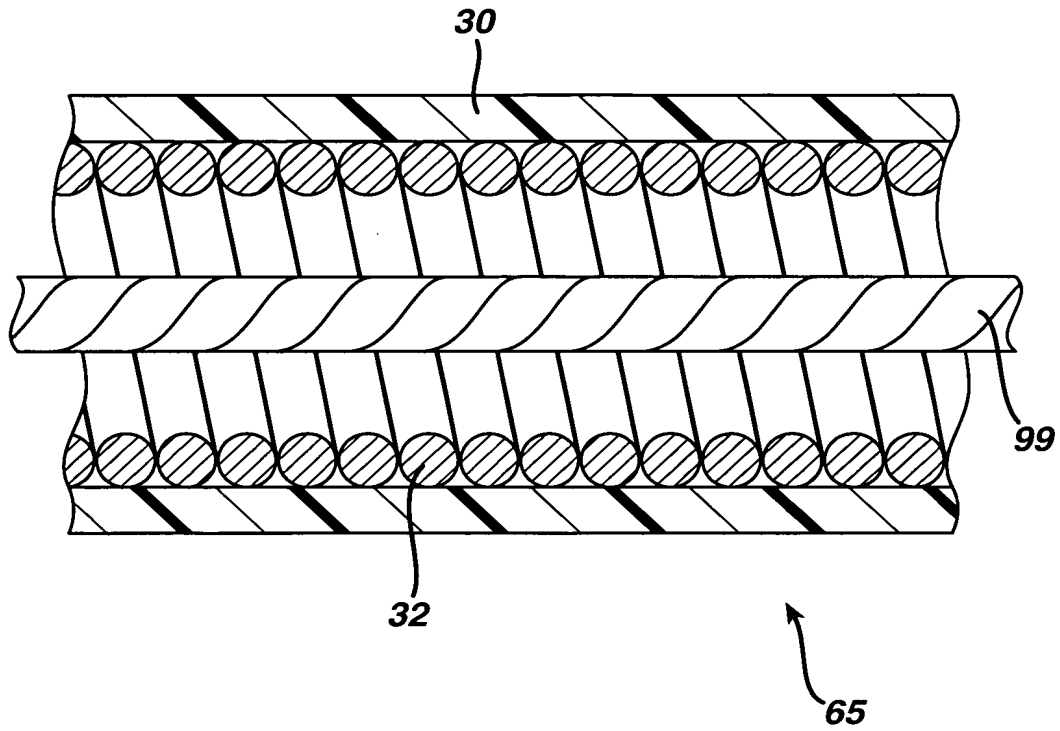


3/14

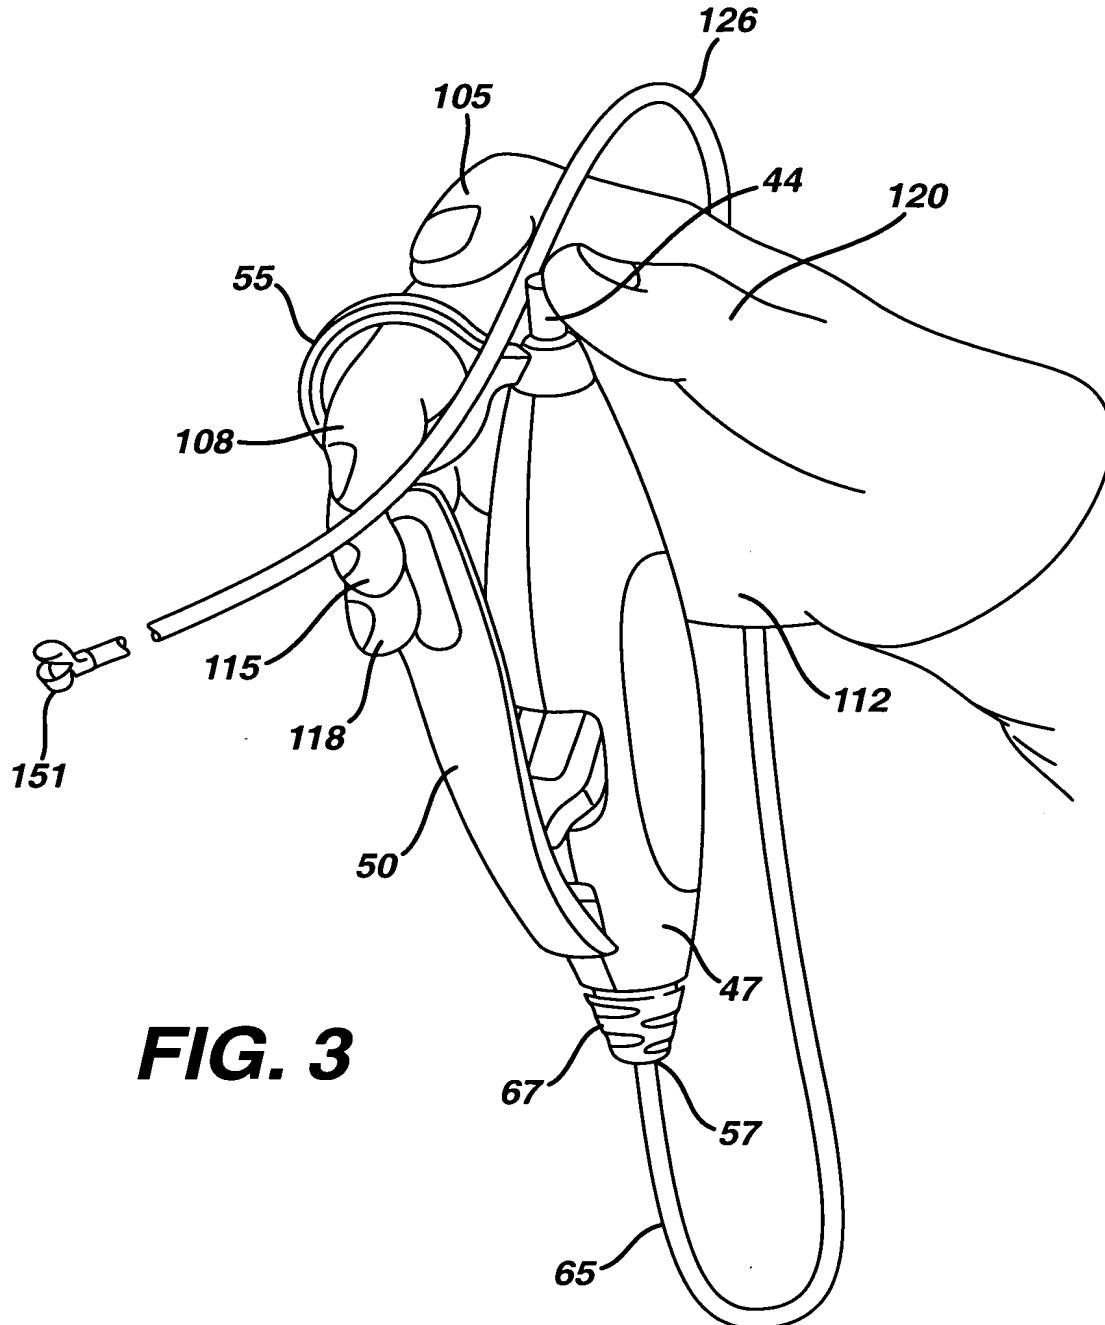

4/14

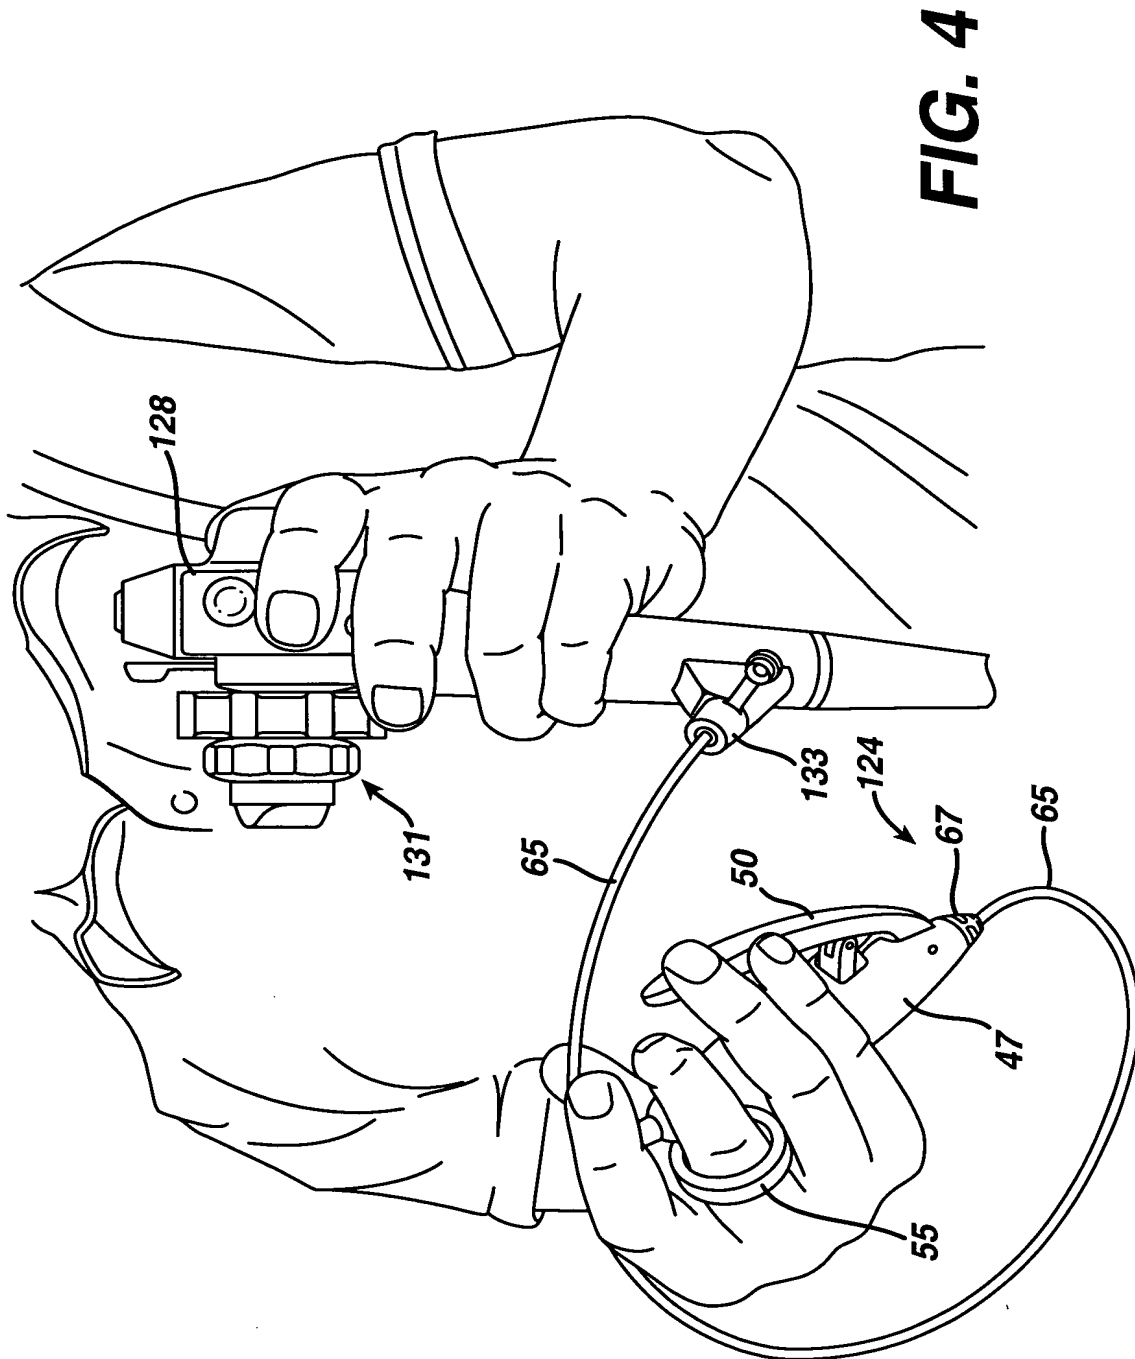

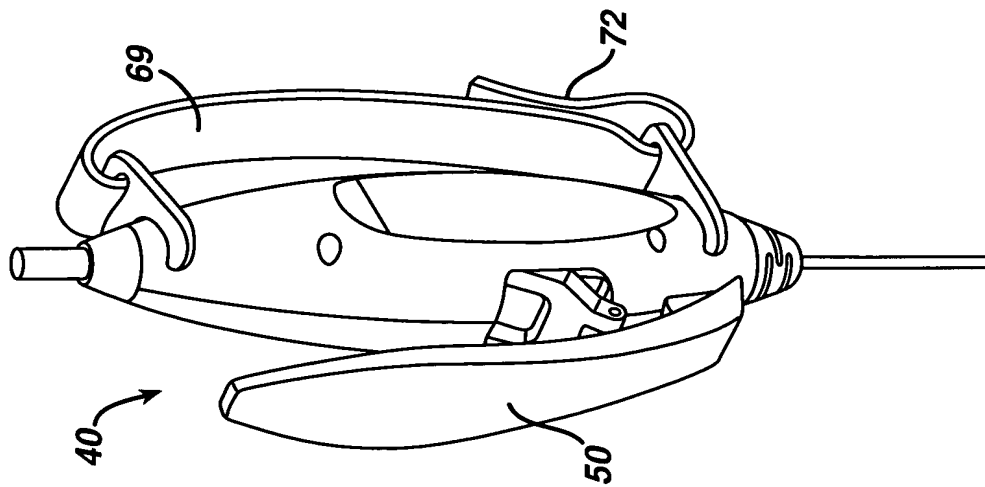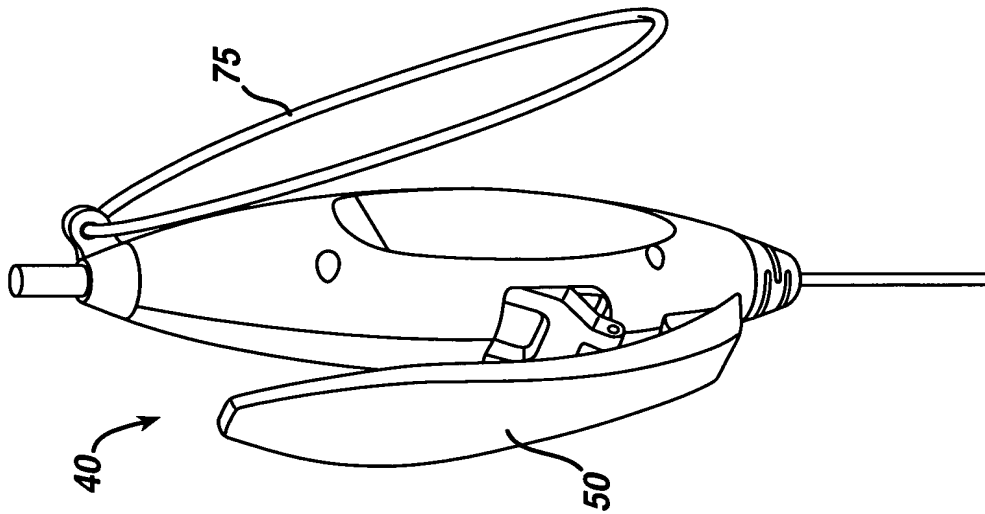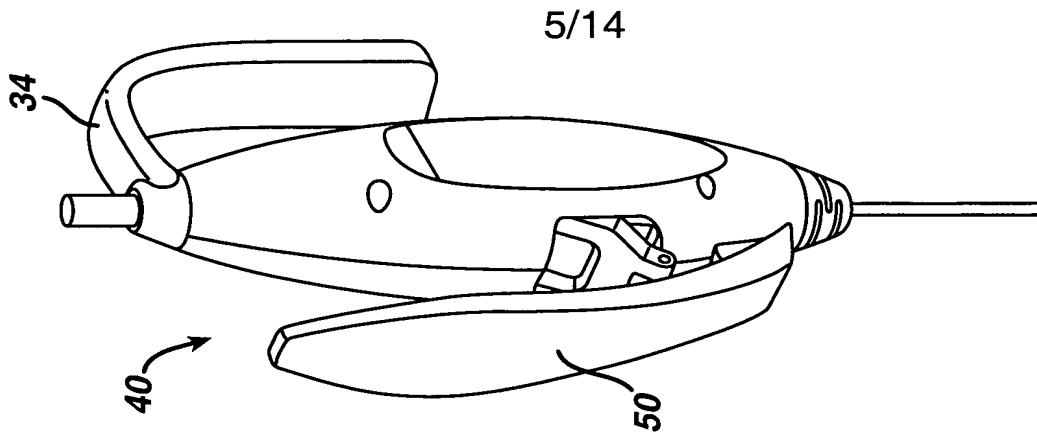

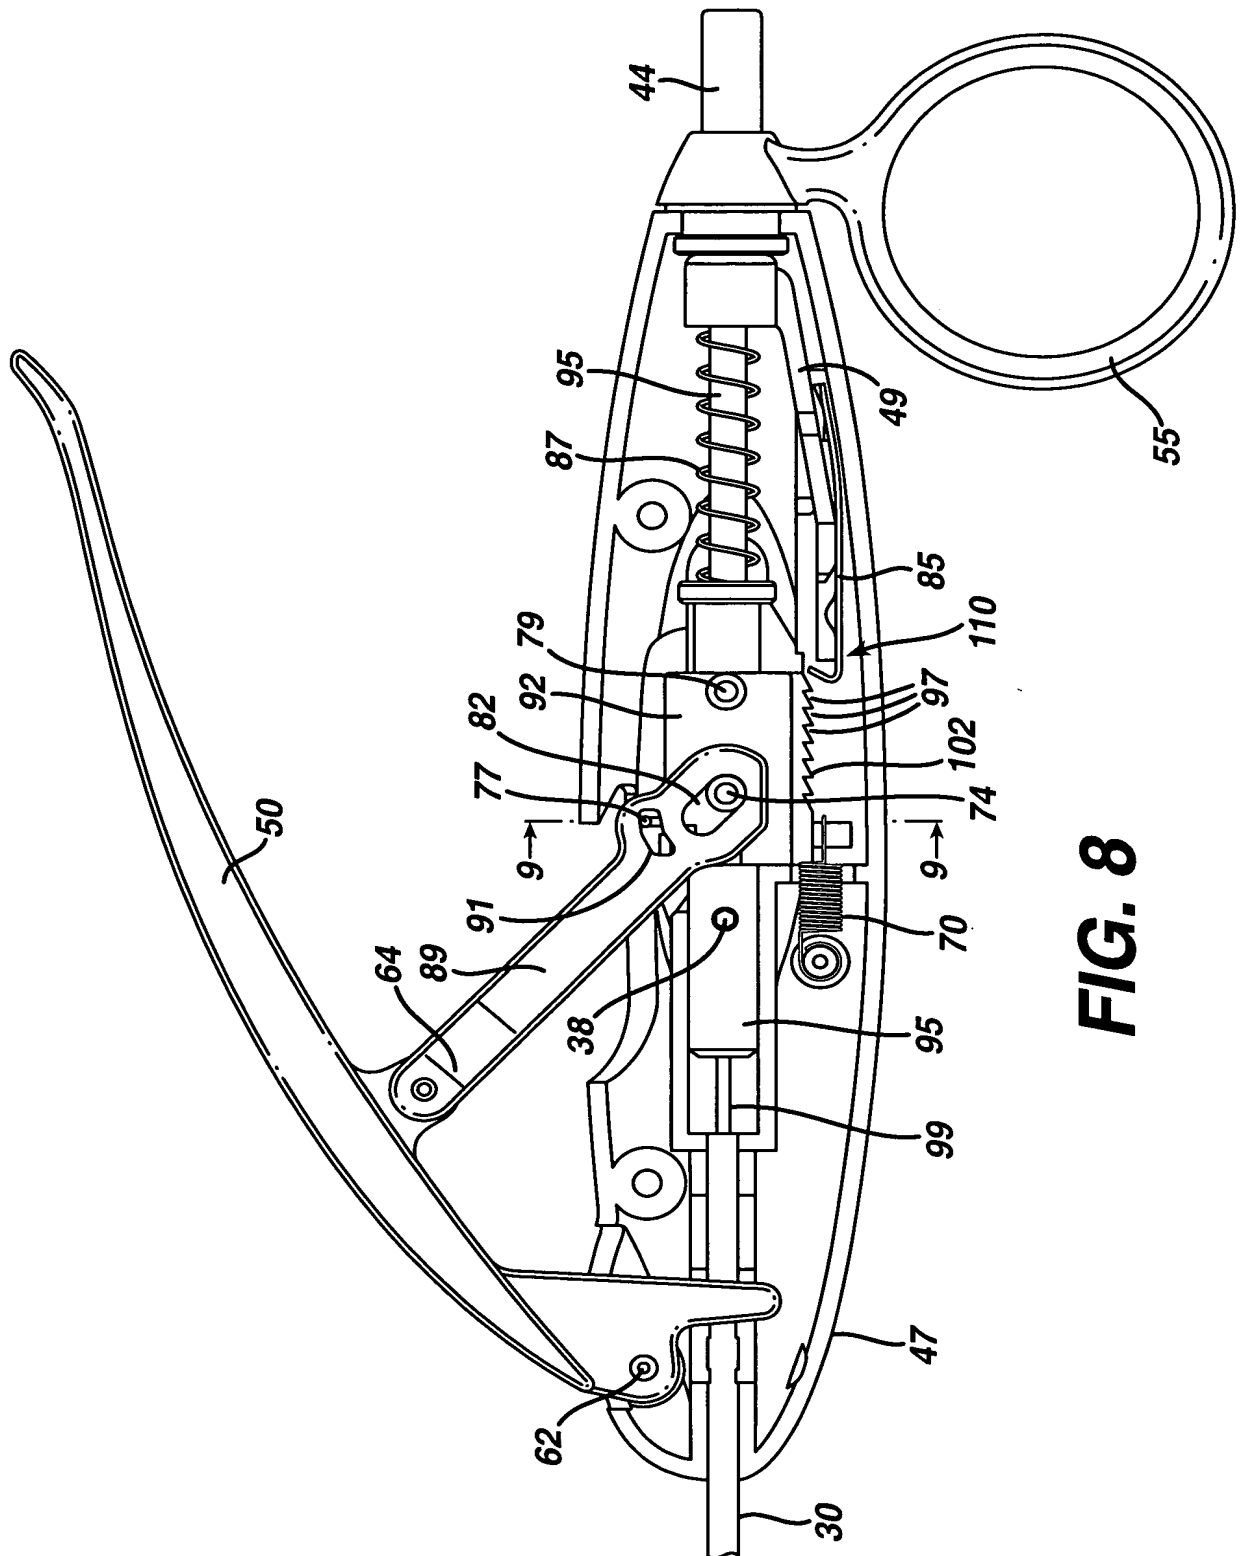


FIG. 8

7/14

FIG. 9


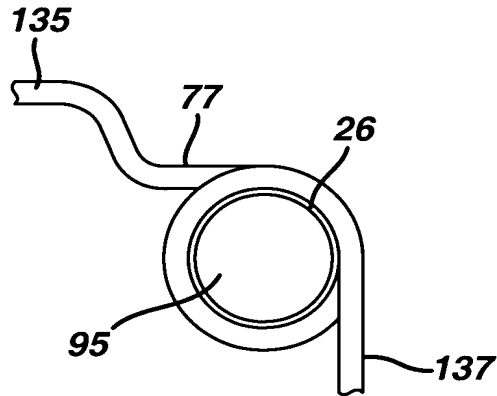


FIG. 11

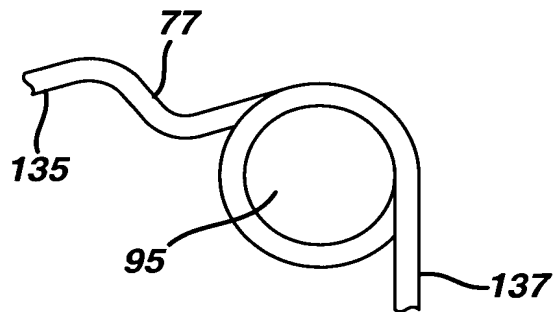

8/14


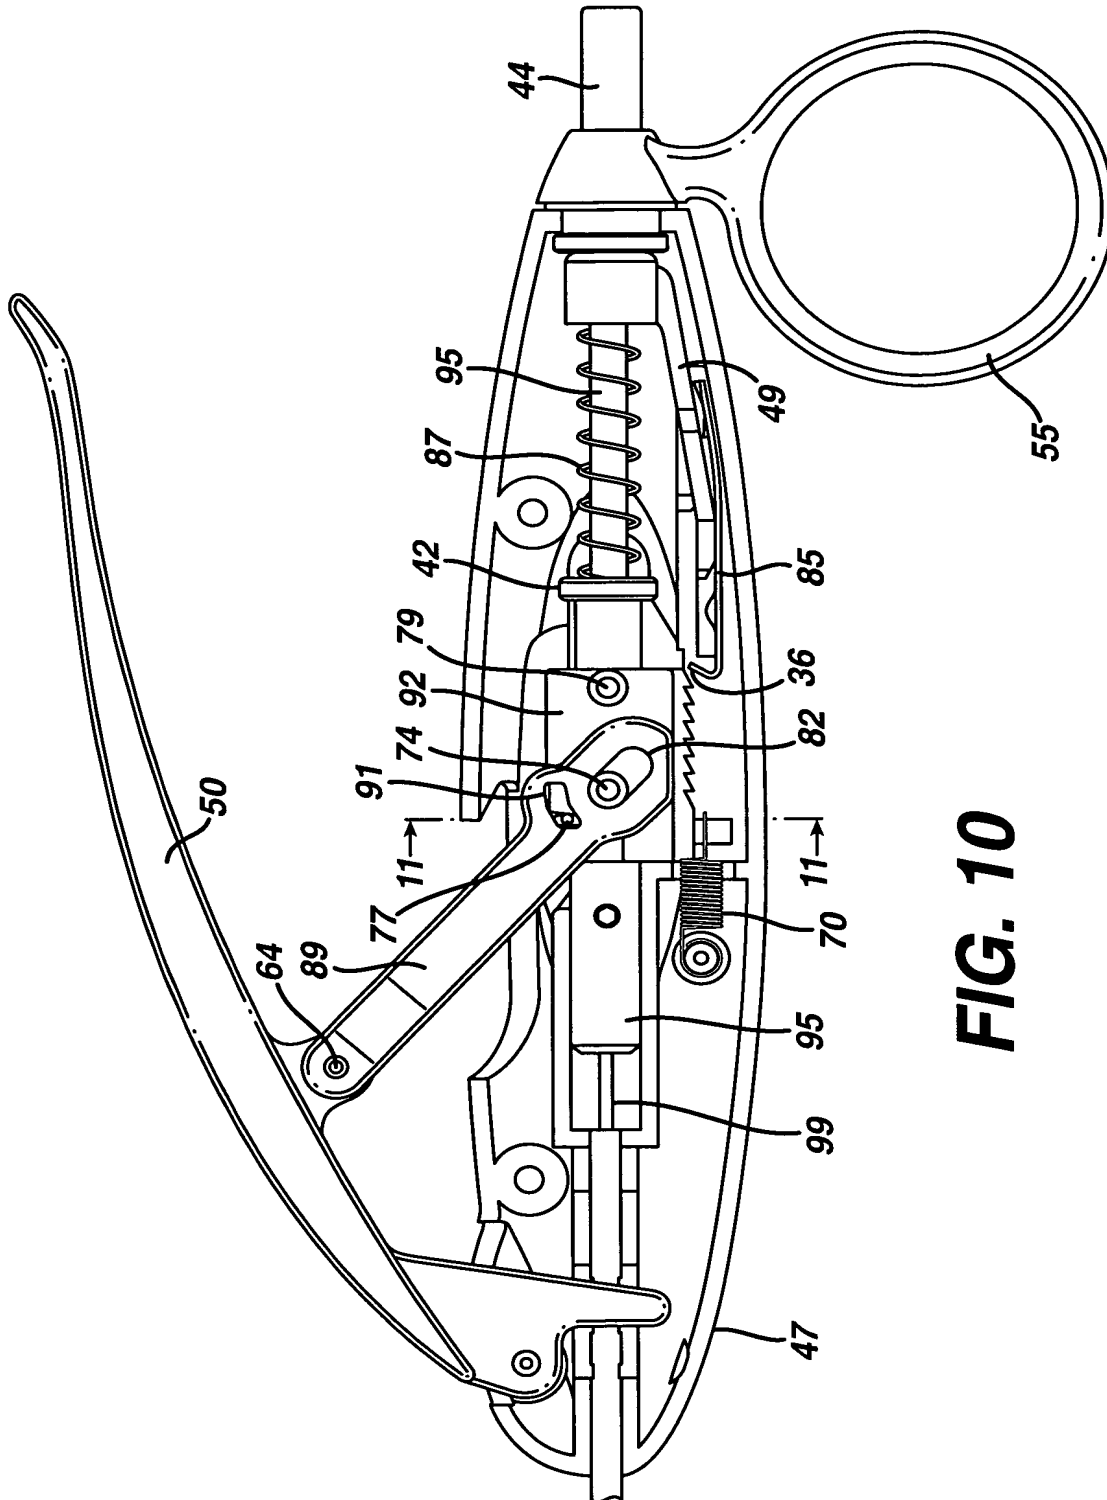


FIG. 10

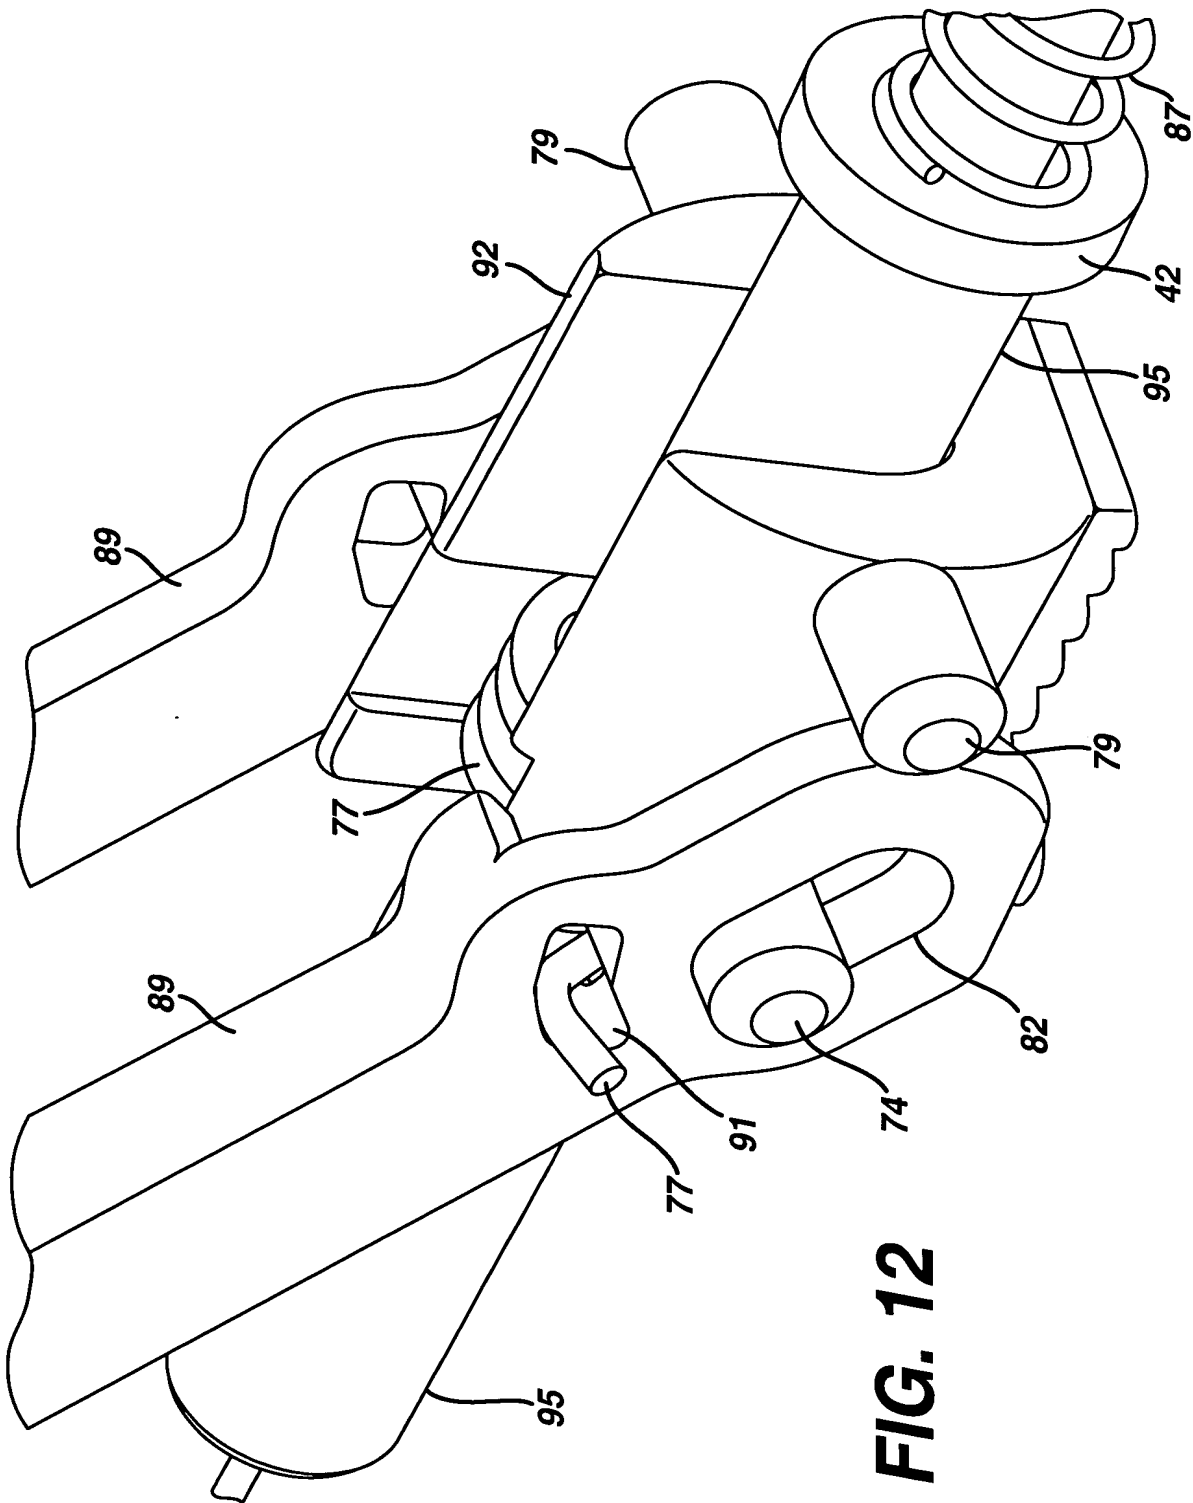

10/14


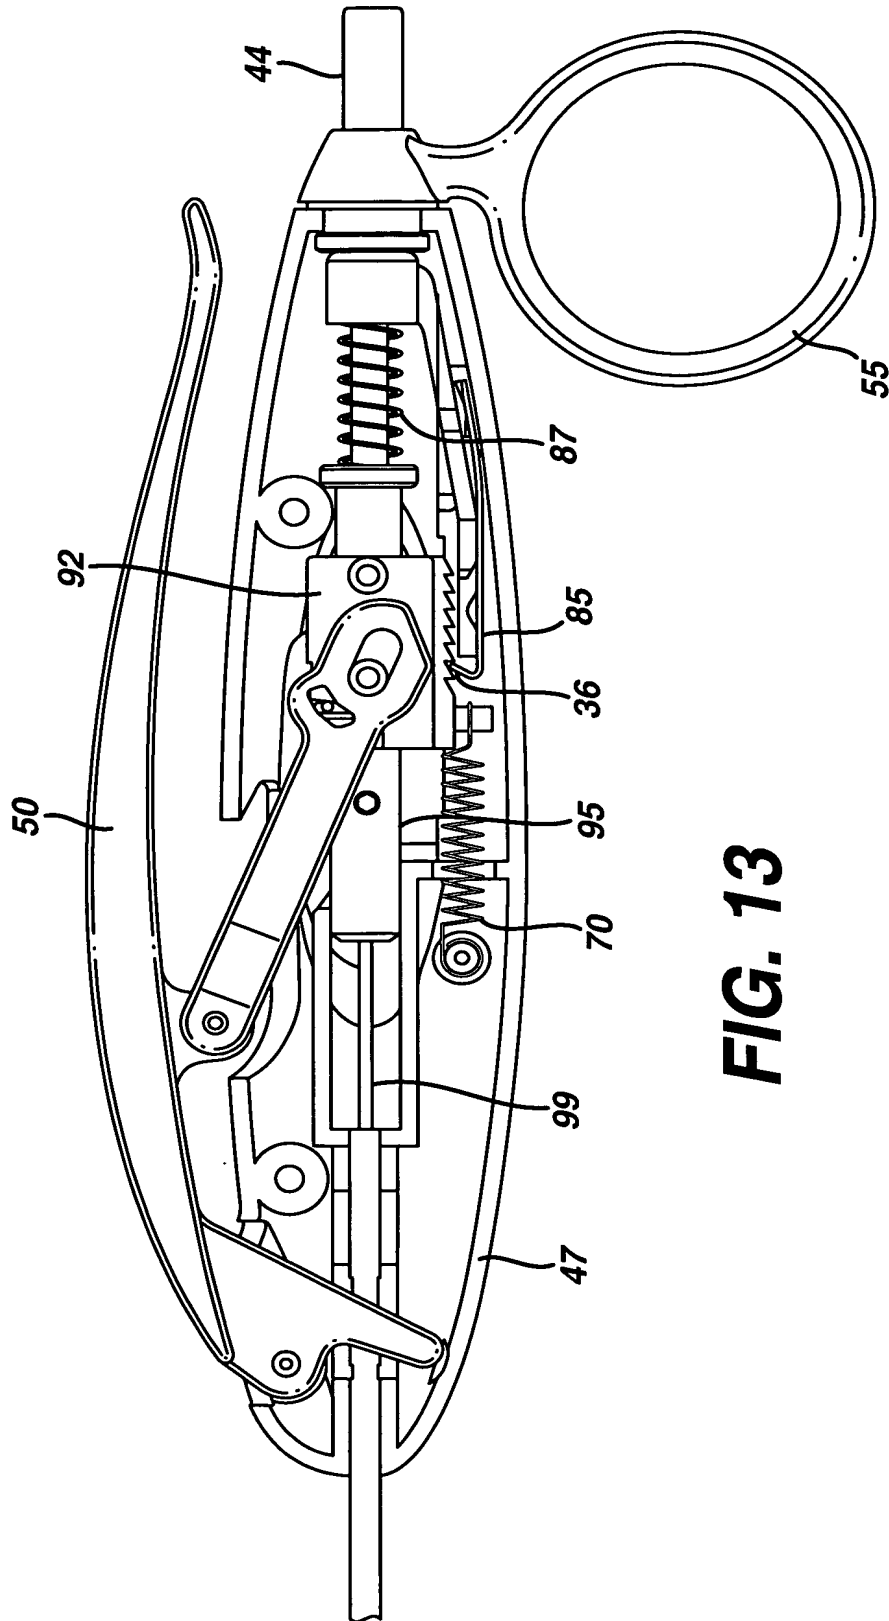



FIG. 13

11/14

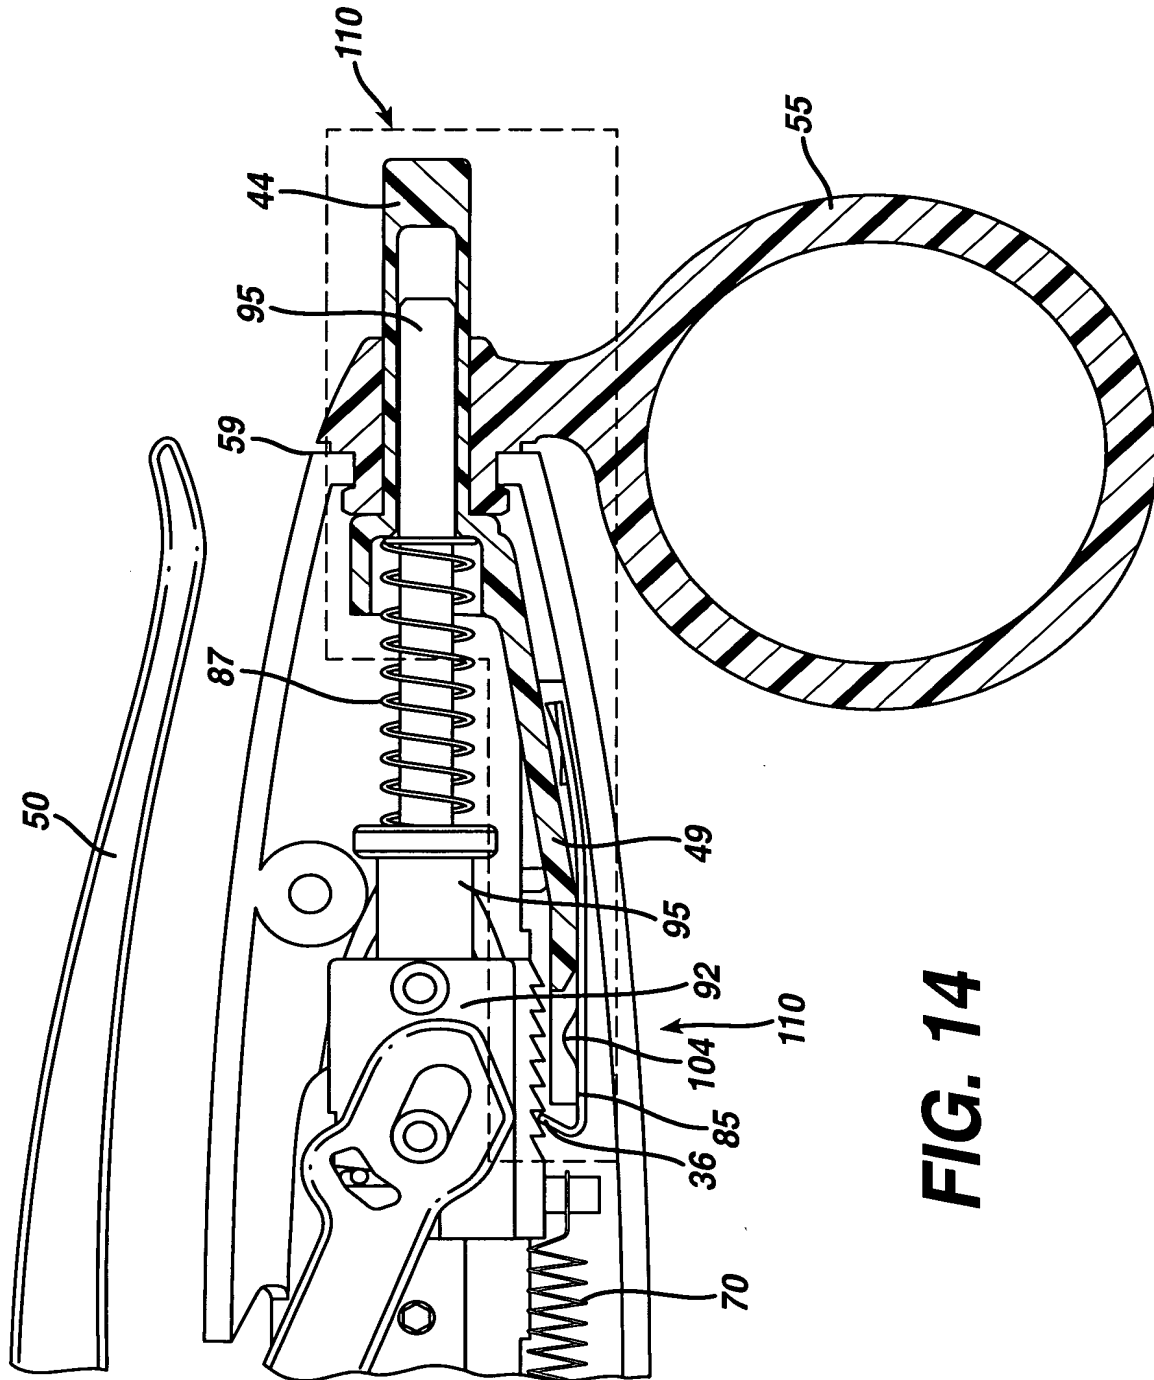


12/14

FIG. 16

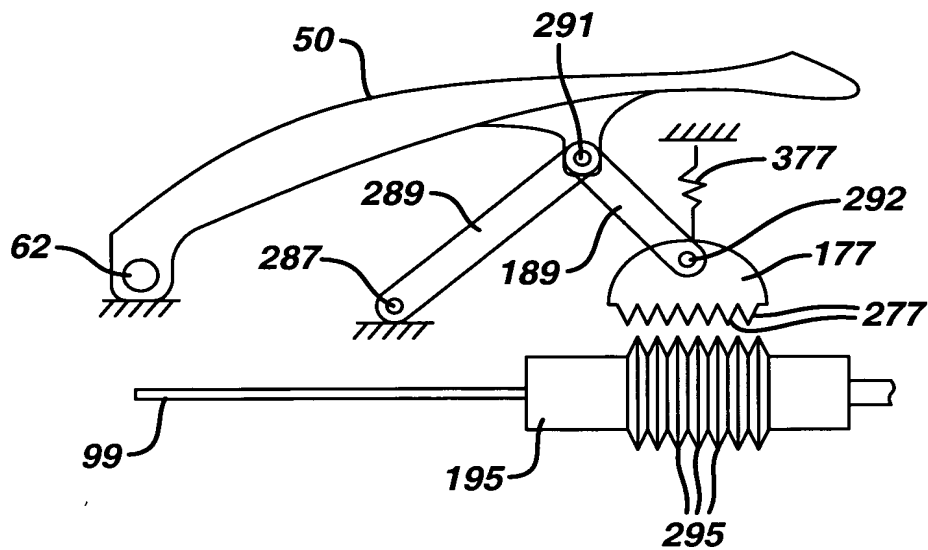

13/14

FIG. 17

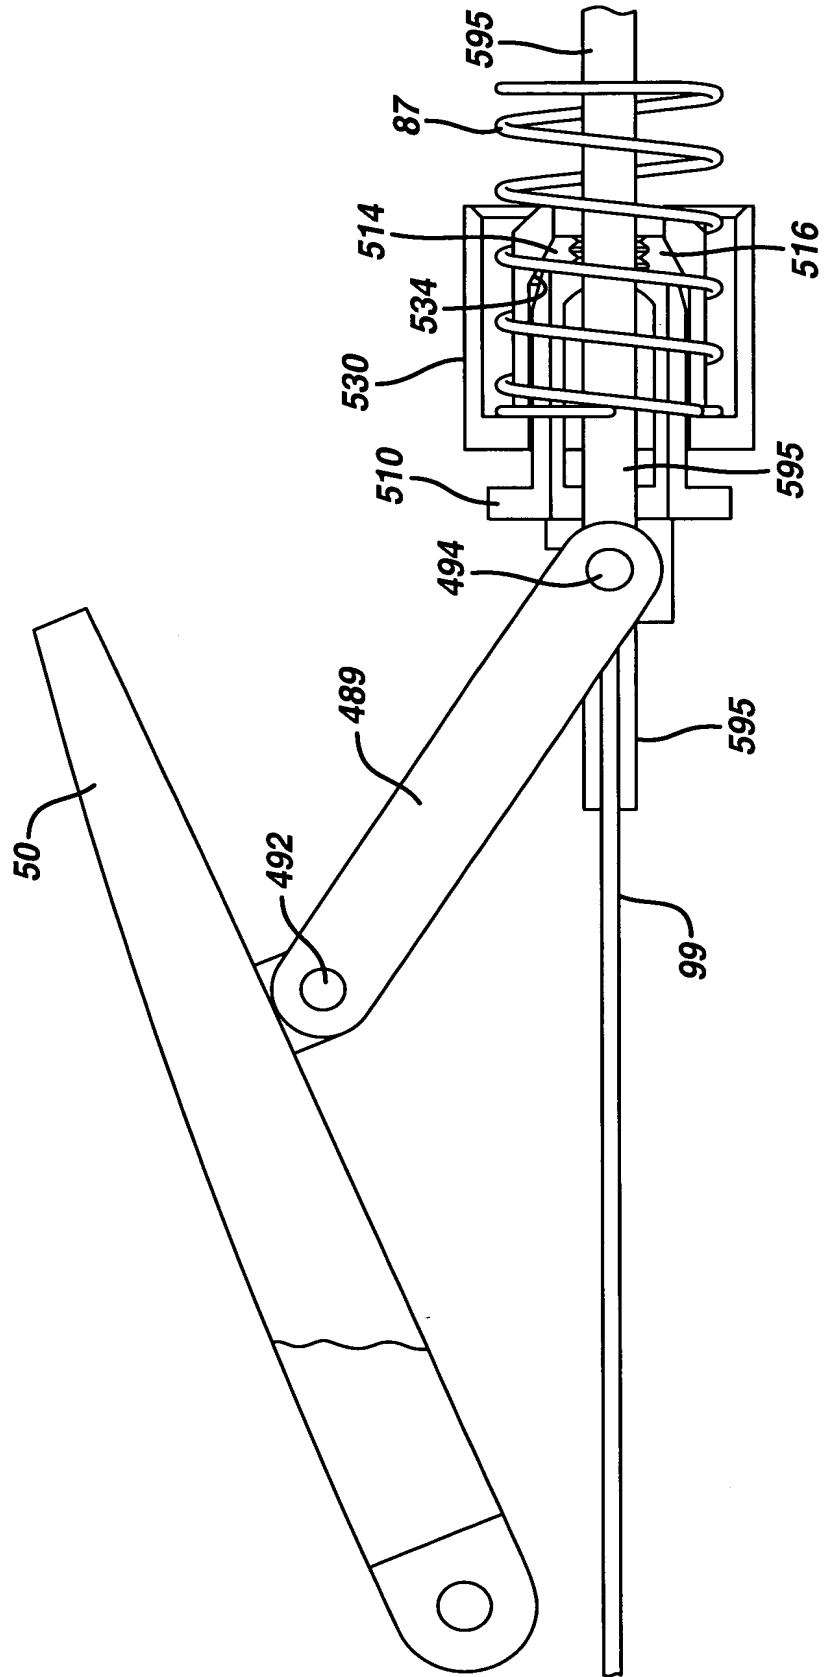

14/14

FIG. 15A




FIG. 15B




FIG. 15C




FIG. 15D




FIG. 15E




FIG. 15F




FIG. 15G




FIG. 15H




FIG. 15I

